

Comparison of lung ultrasound technique *versus* clinical method to evaluate the accuracy of size and placement of left endobronchial double lumen tube in patients undergoing elective thoracic surgery: a prospective observational study

Correspondence: Pooja Singh, Department of Anesthesiology and Critical Care, All India Institute of Medical Sciences, Saket Nagar, 462020 Bhopal, Madhya Pradesh, India.
Tel.: +91.9910838272, +91.9340969292.
E-mail: pooja.anesth@aiimsbhopal.edu.in

Key words: thoracic anesthesia, airway management, endobronchial double lumen tube, tracheal ultrasonography, lung ultrasound, anthropometric measurement, lung isolation.

Contributions: all authors have contributed significantly and agree with the content of the manuscript. PS, EG, experiment concept and design; EG, YN, experiments performing; PS, SJ, RP, SK, literature search; EG, YN, RP, SJ, data acquisition; PS, STK, VW, analysis and interpretation of experiment results; PS, STK, SK, manuscript preparation; STK, VW, manuscript review. All the authors have read and approved the final version of the manuscript and agreed to be accountable for all aspects of the work.

Conflict of interest: the authors declare no conflict of interest.

Ethics approval and consent to participate: the study protocol was approved by the Institutional Human Ethics Committee of All India Institute of Medical Sciences, Bhopal (Protocol No.: IHEC-LOP/2019/MD0084 dated 18/12/2019).

Informed consent: written informed consent was obtained from a legally authorized representative(s) for anonymized patient information to be published in this article. The manuscript does not contain any individual person's data in any form.

Availability of data and materials: all data generated or analyzed during this study are included in this article.

Funding: none.

Received: 5 July 2023.

Accepted: 5 September 2023.

Early view: 18 September 2023.

Publisher's note: all claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers. Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.

©Copyright: the Author(s), 2023

Licensee PAGEPress, Italy

Monaldi Archives for Chest Disease 2024; 94:2700

doi: 10.4081/monaldi.2023.2700

This article is distributed under the terms of the Creative Commons Attribution-NonCommercial International License (CC BY-NC 4.0) which permits any noncommercial use, distribution, and reproduction in any medium, provided the original author(s) and source are credited.

Ekta Gupta,¹ Pooja Singh,¹ Sunaina Tejpal Karna,¹
Yogesh Niwariya,² Vaishali Waindeskar,¹ Sourabh Jain,³
Rajesh Panda,⁴ Sandeep Kumar¹

¹Department of Anesthesiology and Critical Care, All India Institute of Medical Sciences, Bhopal, Madhya Pradesh;

²Department of Cardiothoracic and Vascular Surgery, All India Institute of Medical Sciences, Bhopal, Madhya Pradesh;

³Department of Critical Care, Apollo-Sage Hospital, Bhopal,

Madhya Pradesh; ⁴Department of Critical Care, Kalinga Institute of Medical Sciences, Bhubaneswar, Orissa, India

Abstract

Anthropometric measurements like height and gender have been frequently found to be inaccurate in the prediction of the size of double lumen tube (DLT). Tracheal ultrasonography is a technique that can be used to predict the size of DLT and its correct placement for lung isolation. We aim to check the accuracy of ultrasound over clinical methods. This prospective study included 68 patients undergoing elective thoracic surgery requiring one-lung ventilation with DLT. The groups were assessed for the size of DLT by either anthropometric measurement using height and gender (group C) or ultrasound method (group U). Further, the accuracy of placement of DLT was assessed through either lung auscultation in group C or various ultrasonographic and ventilatory parameters such as lung isolation in the first attempt (lung sliding and lung pulse sign), oxygenation status, and peak airway pressure in group U. Surgeon satisfaction score was also compared in both groups. The accuracy of predicted DLT size between group C and group U was statistically significant ($p=0.044$). In group C, 56% of patients showed a mismatch between the predicted DLT size and the actual size required, while in group U, the mismatch was only 32.4%. The accuracy of DLT placement through group C was 41% as compared to 79% in group U. The surgeon satisfaction score was also significantly higher in group U as compared to group C ($p=0.0028$). Thus, our study suggests that tracheal and chest ultrasonography for DLT size selection and placement for lung isolation is superior to clinical methods.

Introduction

Endobronchial double lumen tube (DLT) is commonly used for lung isolation in patients undergoing thoracic surgeries [1,2]. The selection of appropriately sized DLT is often based on anthropometry-based formulas, chest radiographs, and spiral computed tomography scans. Although pediatric flexible bronchoscopy (FOB) is the

gold standard for confirmation of DLT placement, universal availability of equipment and skilled personnel becomes a limiting factor in a resource-limited area [3-5]. In such scenarios, anesthesiologists rely on clinical methods like auscultation of breath sounds with sequential clamping of both the lumens of DLT or chest radiograph to confirm the correct placement of DLT. However, auscultation may not always recognize the misplacement of DLT, with a reported incidence of 48% by blind methods [3]. A chest X-ray is usually not feasible in intraoperative settings, with the added disadvantage of undue radiation exposure.

Lung ultrasonography (LUS) is a non-invasive, bedside technique, often used to confirm the correct placement of the endotracheal tube and to identify the lung's respiratory movement [6].

There are limited studies on the utility of ultrasound (USG) in confirming the correct size or placement of DLT in resource-limited settings. With this research gap, we undertook this study with the primary objective of evaluating accuracy of trachea and lung USG in assessing the appropriate size and placement of DLT for lung isolation compared to the clinical method. Secondary outcomes were the time required for DLT placement, incidence of respiratory complications, and satisfaction grading of lung isolation by the operating surgeon through direct observation.

Materials and Methods

This was a single-center, prospective, observational cohort study in which consecutive patients aged 18-75 years, of either sex, belonging to American Society of Anesthesiologists physical status I, II or III, scheduled for elective thoracic surgery requiring one-lung ventilation (OLV) with left DLT, were recruited from January 2020 to March 2021 after Institutional human ethical committee approval (IHEC-LOP/2019/MD0084) and registration of the study under the clinical trial registry of India (CTRI/2021/04/042691). Written informed consent was given by all study participants for using anonymized data for scientific purposes. Patients with an anticipated difficult airway, tracheostomy, deranged pulmonary function tests, re-do surgery, and pneumothorax were excluded.

The consecutive patients fulfilling the inclusion and exclusion criteria were assigned alternately to two groups: i) group C – the prediction of left DLT size was based on the anthropometric measurement (height and gender) and assessment of correct placement of DLT was done clinically by the auscultatory method by sequential clamping of both the lumen of DLT; ii) group U – the prediction of left DLT size was done after assessing tracheal width by ultrasonography as suggested by Brodsky *et al.* [7] (Table 1). Correct placement of DLT for lung isolation was done using lung USG.

Tracheal USG was done using a linear transducer of 6-13 MHz of an USG machine (SonoSite-M-Turbo) with the study participants placed in a supine position with a slightly extended head. The scan was performed in a transverse plane with the transducer marker directed toward the patient's right and perpendicular to the skin over the cricoid cartilage. The transverse diameter of the column of air at the cricoid cartilage was measured, which suggests the size of a trachea, and accordingly, the appropriate size of DLT was chosen (Figure 1).

The same USG machine and probe were used for LUS in three steps: i) both lungs were ventilated and confirmed with the "lung sliding sign"; ii) the tracheal lumen was clamped, and only the left lung was ventilated, which was confirmed with a lung sliding sign on the left side and a "lung pulse sign" (signifies the collapse of the lung) on the right side; iii) the same process was repeated after clamping the bronchial lumen.

As per institutional protocol, after ensuring standard monitoring and securing large-bore intravenous access, anesthesia was induced. The trachea was intubated by an anesthesiologist with at least three years of experience with a left-sided DLT based on prediction as per group allocation. Intratracheal placement of DLT was confirmed by an end-tidal carbon dioxide (EtCO₂) monitor. Lung isolation was confirmed as per the methodology of the allocated group.

During bilateral lung ventilation, the lung was ventilated with tidal volume (TV) of 6-7 ml kg⁻¹ with a fractional inspired concentration of oxygen (FiO₂) of 0.5. Once OLV was initiated, the TV was decreased to 4-5 ml kg⁻¹ with positive end-expiratory pressure (PEEP) of 5 cm of H₂O. The respiratory rate was adjusted to maintain EtCO₂ of 35-45 mmHg.

Correct positioning in both groups was also ascertained by normal airway pressure and oxygenation during OLV. The time taken for placement of the DLT was measured from confirmation of tracheal intubation by capnograph after tracheal balloon inflation till the confirmation of satisfactory lung isolation.

Four parameters were assessed for the accuracy of lung isolation: i) lung isolation achieved at the first attempt; ii) normal peak airway pressure, which is defined as <35cm H₂O; iii) adequate oxygenation status defined as no need for intervention like continuous positive airway pressure, increments in FiO₂ of more than 0.5 or PEEP of more than 5 cm of water to maintain saturation of more than 92%; iv) assessment grading was given by the operating surgeon (as "poor," "good," and "excellent") by direct visualization of intraoperative lung isolation.

If at any point after DLT placement, there was a rise in airway pressure, inadequate oxygenation status, and/or poor surgeon's sat-

Table 1. Choice of the double lumen endobronchial tube according to tracheal width.

Measured tracheal width (mm)	Predicted DLT size (Fr)
>18	41
>16	39
>15	37
<14	35

DLT, double lumen tube.

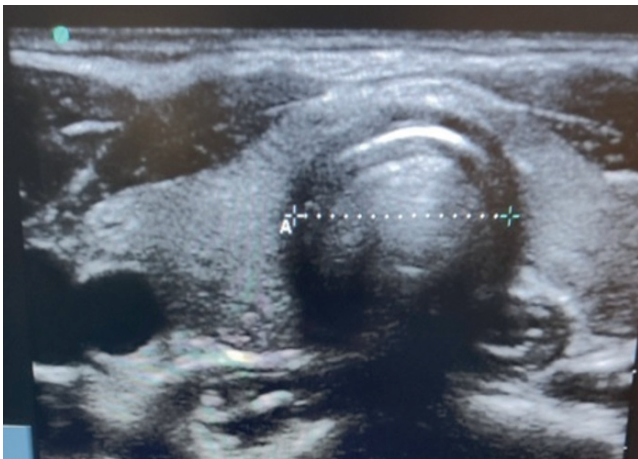


Figure 1. Sonographic image of tracheal diameter measurement at the level of cricoid cartilage.

isfaction score, malposition of DLT was ruled out by intraoperative FOB-guided readjustment, with documentation of the same.

Statistical analysis

PASS 14 Power Analysis and Sample Size Software (NCSS, LLC, Kaysville, UT, USA) was used to determine the sample size with a 95% confidence interval and 80% power. Our sample size was 68 and with a 10% dropout rate, a total of 75 study participants were needed. Microsoft Excel and EPI-info version 7 software (Center of Disease Control and Prevention, Atlanta, GA, USA) were used for data entry and analysis, respectively. Mean and standard deviation summarize numerical data when normally distributed, and count and percentage for summarizing nominal data. Contingency tables were prepared for the data. Categorical data was compared using the Fischer exact test and Pearson Chi-square test. Continuous data was compared using unpaired *t*-test. The p-value, sensitivity, specificity, and accuracy of each group were calculated using the

receiver operating characteristic area under the curve. A p-value of <0.05 was considered as significant.

Results

A total of 75 patients were enrolled in the study. However, 7 patients were excluded, and final data analysis was done in 68 patients (group C=34; group U=34) (Figure 2). Participants in groups C and U were similar in terms of age, sex and height (Table 2).

Double lumen tube size

In group C, estimated DLT size matched with the actual size requirement in 15 patients (44.0%). It was larger and smaller than that predicted in 8 (23.5%) and 11 (32.5%) patients, respectively. Thus, 56% of patients in group C showed a mismatch between the predicted and required DLT size. On tracheal USG, the mean tra-

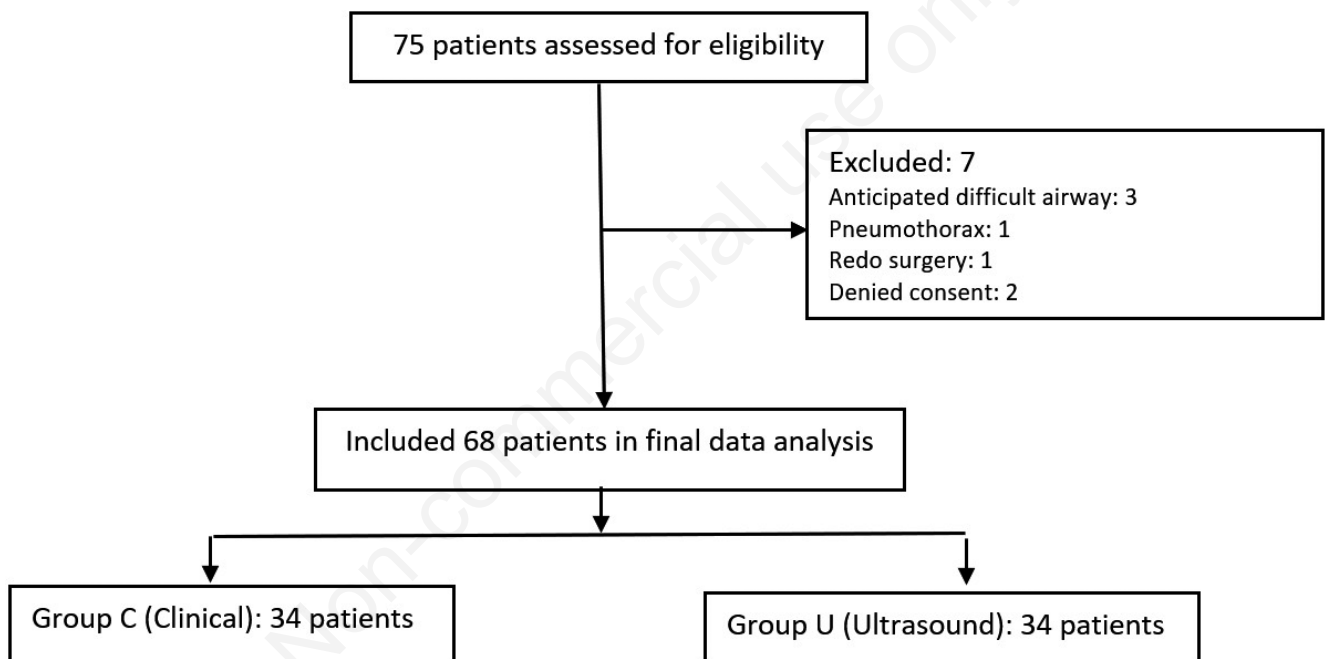


Figure 2. Diagram depicting flow of patients.

Table 2. Demographic characteristics in both groups.

Parameter	Group C	Group U	p
Age (years)	32.77±14.25	34.77±14.36	0.566*
Gender (M/F)	22/12	25/9	0.431 [#]
Height (female) [°]			
<160 cm	9 (75)	5 (55.6)	0.397
>160 cm	0	1 (11.1)	0.429
<152 cm	3 (25)	3 (33.3)	1.00
Height (male) [°]			
<170 cm	17 (77.3)	17 (68)	0.530
>170 cm	0	0	1.00
<160 cm	5 (22.7)	8 (32)	0.530

M/F, male/female. Data expressed as mean±standard deviation; n (%); *unpaired *t*-test; [#]Pearson chi-square test; [°]Fisher's exact test; p<0.05 is significant.

cheal width in males and females was observed as 15.85 and 14.56 mm, respectively (Figure 3). In group U, DLT size matched the actual size requirement in 23 (67.6%) patients. DLT size was larger and smaller than predicted in 5 (14.7%) and 6 (17.6%) patients, respectively. Thus, 32.4% of patients in group U showed a mismatch between the predicted and required DLT size. A statistically significant higher accuracy in predicting DLT size was observed in group U as compared to group C ($p=0.044$) (Table 3).

Double lumen tube placement

Successful lung isolation was achieved on the first attempt in 21 (61.8%) and 29 (85.3%) study participants in groups C and U, respectively ($p=0.028$). The mean peak pressure was observed to be higher in group C as compared to group U (16.21 ± 0.98 vs. 15.00 ± 0.82 ; $p=0.00001$). Three patients (8.8%) in group C had an oxygen saturation of less than 92%, while in group U, there were none ($p=0.239$). FiO_2 more than 0.5 was needed to maintain a saturation of 92% in 16 (47.1%) and 10 (29.4%) patients in group C and group U, respectively, though it was statistically insignificant ($p=0.212$).

Sensitivity, specificity, and predictive value

The sensitivity of lung USG (86%) was significantly higher compared to clinical methods (52%) for the assessment of DLT size, though the specificity of both methods was low (25% and 18%, respectively). The overall accuracy for confirmation of correct DLT

placement of clinical methods (41%) was lower as compared to lung USG (79%) (Table 4).

Complications with double lumen tube placement

In group C, 7 (20.6%) patients had sore throat, compared to 4 (11.8%) patients in group U. Though the difference was statistically insignificant, the USG group had fewer complications. Trauma during intubation was not seen in any of the two groups. More than one intubation attempts were seen in 13 (38.2%) and 5 (14.7%) patients in group C and group U, respectively ($p=0.0028$) which was attributable to improper tube size.

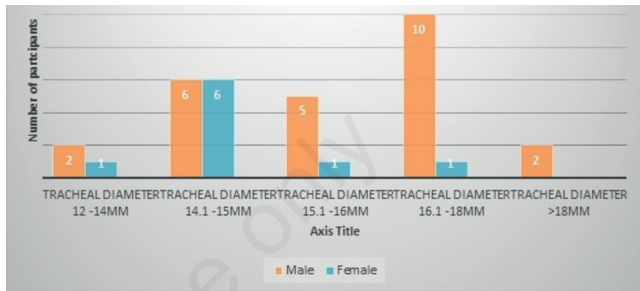


Figure 3. Distribution of tracheal width in the ultrasound (USG) group.

Table 3. Difference in double lumen tube size in both the groups.

Actual DLT used	Group 1		Group 2		Z test
	n	%	n	%	
Same as predicted	15	44.0	23	67.6	$Z=-2.01, p=0.044$
Higher than predicted	8	23.5	5	14.7	
Lower than predicted	11	32.5	6	17.6	
Total	34	100.0	34	100.0	

DLT, double lumen tube.

Table 4. Parameters assessed for adequacy of lung isolation, surgeon satisfaction score, the time required for double lumen tube (DLT) placement and complications of DLT placement.

Parameter	Group 1	Group 2	p^*	p
Lung isolation				
Lung isolation achieved at first attempt	21 (61.8)	29 (85.3)	0.028	-
Peak pressure	16.21 ± 0.98	15.00 ± 0.82	-	0.0001 [#]
Oxygenation status Saturation (less than 92%)	3 (8.8)	0	0.239	-
FiO_2 (more than 0.5) to maintain saturation 92%	16 (47.1)	10 (29.4)	0.212	-
Surgeon satisfaction score				
Poor	2 (5.9)	1 (2.9)	-	0.0028 ^o
Acceptable	20 (58.8)	7 (20.6)		
Excellent	12 (35.3)	26 (76.8)	-	
Time required for confirmation of position of DLT from intubation				
0-4 minutes	12 (35.3)	31 (91.2)	<0.0001	-
4.1-8 minutes	22 (64.7)	3 (8.8)		
Complications				
Sore throat	7 (20.6)	4 (11.8)	-	0.512 [§]
Trauma during intubation	0	0	-	1.0 [§]
More than one intubation attempt	13 (38.2)	5 (14.7)	-	0.028 [§]

Data expressed as mean±standard deviation, n (%). FiO_2 , fractional inspired oxygen concentration; DLT, double lumen tube; *Fisher's exact test; [#]unpaired t -test; ^oPearson Chi-square test; [§]Chi-square test.

Table 5. Sensitivity, specificity, and predictive value of clinical and ultrasound to predict size and accuracy of placement of double lumen tube.

Parameter	Group C			Group U		
	Value (%)	CI-lower limit (%)	CI-upper limit (%)	Value (%)	CI-lower limit (%)	CI-upper limit (%)
Sensitivity	52.17	30.59	73.18	86.67	69.28	96.24
Specificity	18.18	2.28	51.78	25	0.63	80.59
PPV	57.14	45.20	68.31	89.66	82.87	93.95
NPV	15.38	4.61	40.60	20	3.51	63.20
Accuracy	41.18	24.65	59.30	79.41	62.10	91.30

CI, confidence interval; PPV, positive predictive value; NPV, negative predictive value.

Surgeon satisfaction score and rapidity of placement

In group C, surgeons gave an acceptable and excellent satisfaction score in 20 (58.8%) and 12 (35.3%) patients, respectively. Poor satisfaction score was observed in 2 (5.9%) patients. In group U, surgeons gave an excellent and acceptable satisfaction score in 7 (20.6%) and 26 (76.5%) patients, respectively. A poor satisfaction score was seen in one (2.9%) patient only. The association between the surgeon satisfaction score and the groups was significant ($p=0.0028$). The mean duration from intubation to placement confirmation was significantly higher in group C as compared to group U (250 vs. 192 sec, $p<0.0001$) (Table 5).

Discussion and Conclusions

In this prospective observational cohort study of 68 patients undergoing elective thoracic surgery requiring OLV, we found that USG had higher accuracy in the prediction of DLT size than anthropometric formula-based methods. Lung USG fared better in diagnostic accuracy, with higher sensitivity and surgeon satisfaction scores and faster confirmation of correct DLT placement.

Size of double lumen tube

The optimal size DLT is the largest tube whose main body passes through the glottis without any trauma while the bronchial lumen fits the desired bronchus with only a small air leak when its cuff is deflated [8]. An inappropriately sized DLT can interfere with oxygenation, cause airway trauma, and affect lung isolation during OLV [9]. The demographic parameters such as height and gender-based formulas used to predict the DLT size, may not be accurate, especially in Asians, who are generally smaller [8,10]. Brodsky *et al.* found that the average tracheal widths for Asian and non-Asian men were 19 ± 2 mm and 21 ± 2 mm, whereas that for women were 16 ± 2 mm and 17 ± 3 mm, respectively [8].

In a previous study, the width of the trachea was measured in 70 patients at the level of the clavicles in a recent posteroanterior chest radiograph. They found average tracheal diameter for males was 22 mm (range 15-27 mm) and 17 mm (range 13-25 mm) in females [7]. However, in the present study, the average tracheal diameter in males and females was 15.85 mm (range 13-20 mm) and 14.56 mm (range 12.5-16 mm), respectively. The difference in the measured tracheal diameter can be due to different population characteristics of different areas. Further, in our study, the tracheal diameter was measured at the level of the cricoid cartilage, while Brodsky *et al.* measured the tracheal diameter at the level of the clavicle.

Considering anthropometric measurements of the Indian population, a DLT size of 39 Fr and 37 Fr are usually chosen for adult males and females, respectively. When assessed through the USG

method, we could place a 41 Fr tube in two adult males, 35 Fr in one adult male, and 32 Fr in one adult female, using the tracheal diameter as a guide. Such varied size prediction is not possible with clinical methods, which ultimately causes difficulty in achieving proper lung isolation due to inappropriate-sized DLT. On the other hand, measurement of tracheal diameter with the help of the USG technique reduces the chances of inappropriate DLT insertion and time duration of DLT placement from intubation to tube fixation with the better achievement of OLV [11].

Direct measurement of tracheal width by imaging modalities like chest radiographs or USG can be used to help predict the optimal size of DLT, independent of height and gender [10,12]. Due to lateral positioning in thoracotomy, an undersized DLT may easily advance too deep into the bronchus and obstruct the upper lobe orifice. In such cases, inflation of the bronchial cuff with a larger air volume could lead to cuff herniation or cuff rupture. If underinflated, the lungs will fail to collapse with unsuccessful lung isolation. The lumen of smaller DLT offers more resistance to airflow during OLV and makes it more challenging to advance the suction catheter and FOB. Conversely, if an oversized DLT is used, it may injure the airway [13]. Significantly better accuracy of the USG technique was observed in predicting the optimum size of DLT as compared to the clinical method. Moreover, measurements are reproducible, with the benefit of no radiation exposure to the patients.

Confirmation of double lumen tube placement

Clinical confirmation of proper DLT placement is done by inspecting chest wall movements and auscultating breath sounds. However, it is non-specific and less accurate [14]. Auscultation depends on the sensitivity of the stethoscope, hearing acuity of the individual, TV, thickness of the chest wall, consistency of underlying lung tissue, and extent of underlying lung pathology. Conductance of sound from the other side of the chest confounds the auscultation of one side of the chest [14].

USG is a non-radiation, non-invasive, easy-to-learn, and quick technique, often available in operation theatres. Limited studies have used sonographic prediction of DLT size and lung sliding sign in confirming the position of DLT [7]. The concept of lung sliding, the sonographic observation of the movement of the visceral pleura against the parietal pleura, was first introduced by Lichtenstein in 1980 [15]. It depends on compliance and TV and can be used for continuous ventilation monitoring. The accuracy of lung USG can be enhanced with the M-mode found on most USG machines [16]. In M-mode, the presence of the lung sliding sign is visualized as the seashore sign, and the absence of lung sliding can be seen as the stratosphere sign [17]. In the non-ventilated or collapsed lungs, a lung sliding sign is absent, and the pleural line moves with heartbeats in a pulsatile manner known as the lung pulse sign. Lung pulse sign is 93% sensitive and 100% specific in identifying lung collapse

[15]. Thus, if a sonographic demonstration of lung sliding on one side and lung pulse on the other side of the chest is present, then adequate functional lung isolation can be predicted [8]. Sustic *et al.* have emphasized adding a brief USG examination to clinical assessment to increase the ability to confirm the placement of DLT [18]. In our study, a significantly higher success rate of identification of lung isolation was achieved at the first attempt in the USG group than in the clinical group ($p=0.0028$). The average time required to achieve lung isolation was considerably lower in the USG (192 sec) technique than in clinical methods (250 sec).

The adequacy of lung isolation does not rule out the advancement of the bronchial lumen beyond the secondary carina. Such advancement would result in poor oxygenation, increased airway pressure, or both [8]. So, in addition to functional lung isolation by USG, if the patient's airway pressure and oxygenation status are within normal limits during OLV, then one can safely comment that the DLT position is satisfactory. Brodsky *et al.* described that if DLT is in the correct bronchus with effective lung isolation, and there is no deoxygenation due to malposition, the position of DLT is commented as 'satisfactory,' and FOB need not be a routine part of DLT placement [7].

In our study, though the difference in the mean peak airway pressure between the two groups showed statistical significance, clinical relevance was not seen. However, the result interpretation showed the superiority of the USG group compared to the clinical group with regards to FiO_2 requirement and frequency of patients who desaturated.

Alvarez-Diaz *et al.* showed that 84.5% sensitivity and 41.1% specificity of the clinical method for accurate placement of DLT in a study on 105 patients [19]. In contrast, USG had a much higher sensitivity of 98.6% and specificity of 52.9%. Saporito *et al.* found that thoracic USG done by a trained nurse anesthetist can be as specific and sensitive as FOB in confirming DLT position [20]. Lung USG was more rapid and cost-effective than FOB in confirming DLT placement. Therefore, it can be suggested that though FOB is a standard gold method in determining precise DLT placement, LUS can be used as a better complementary method to FOB than auscultation in terms of its ability to confirm functional lung isolation [6,12]. In our study, compared to a clinical method, LUS had higher sensitivity and specificity for accurate placement of DLT. Further, the surgeon satisfaction score was excellent in 26 (76.5%) group C, 12 (35.3%) patients had excellent scores and in group U, patients had excellent scores ($p=0.0028$).

Due to undersized or oversized tubes, multiple attempts, and inadequate lubrication, several complications, such as sore throat and airway trauma, can occur. We observed a lesser incidence of sore throat in the USG group, though it did not achieve statistical significance. This may be attributed to the selection of the appropriate size.

Strengths and limitations of the study

This is a prospective study in which we have independently assessed the accuracy of two techniques. We have focused more on the adequacy of functional isolation of the lungs through airway pressure and FiO_2 requirement, which is critical in thoracic surgery. The final assessment of the placement of DLT was done through direct visualization by surgeon satisfaction score, which was not much used previously.

Our study has many limitations. First, consecutive patients were selected, and group allocation was based on the opinion of the consultant anesthesiologist. Randomization was not done. Second, ultrasonography is also a skill-based technique with the possibility

of inter-individual variation during interpretation. Third, lung USG may be unreliable when precise positioning of DLT is mandatory, like broncho-alveolar lavage or massive hemoptysis. In conditions such as surgical pleurodesis or post-inflammatory pleural adhesions, mesothelioma, the lung sliding sign will be absent. It will also be absent during exacerbation of chronic obstructive pulmonary disease, due to hyperinflation of the lung [13]. Therefore, such conditions must be taken into account before using LUS.

The prediction of DLT size by measuring tracheal diameter through USG has significantly improved the selection of appropriate DLT size. Using lung USG alone or in conjunction with clinical methods also improves the accuracy of confirming functional lung isolation. Further randomized studies are warranted to confirm the findings of our study.

References

1. Bahk JH, Lim YJ, Kim CS. Positioning of a double-lumen endobronchial tube without the aid of any instruments: an implication for emergency management. *J Trauma* 2000;49:899-902.
2. Moloney JT, Fowler SJ, Chang W. Anesthetic management of thoracic trauma. *Curr Opin Anaesthesiol* 2008;21:41-6.
3. Smith GB, Hirsch NP, Ehrenwerth J. Placement of double-lumen endobronchial tubes. Correlation between clinical impressions and bronchoscopic findings. *Br J Anaesth* 1986;58:1317-20.
4. Cohen E. Double-lumen tube position should be confirmed by fiberoptic bronchoscopy. *Curr Opin Anaesthesiol* 2004;17:1-6.
5. Klein U, Karzai W, Bloos F, et al. Role of fiberoptic bronchoscopy in conjunction with the use of double-lumen tubes for thoracic anesthesia: a prospective study. *Anesthesiology* 1998;88:346-50.
6. Weaver B, Lyon M, Blaivas M. Confirmation of endotracheal tube placement after intubation using the ultrasound sliding lung sign. *Acad Emerg Med* 2006;13:239-44.
7. Brodsky JB, Macario A, Mark JB. Tracheal diameter predicts double-lumen tube size: a method for selecting left double-lumen tubes. *Anesth Analg* 1996;82:861-4.
8. Brodsky JB, Lemmens HJ. Tracheal width and left double-lumen tube size: a formula to estimate left-bronchial width. *J Clin Anesth* 2005;17:267-70.
9. Eldawlatly AA. Double lumen tube: size and insertion depth. *Saudi J Anaesth* 2021;15:280-2.
10. Zhang C, Qin X, Zhou W, et al. Prediction of left double-lumen tube size by measurement of cricoid cartilage transverse diameter by ultrasound and CT multi-planar reconstruction. *Front Med* 2021;8:657612.
11. Chow MY, Liam BL, Lew TW, et al. Predicting the size of a double-lumen endobronchial tube based on tracheal diameter. *Anesth Analg* 1998;87:158-60.
12. Parab SY, Kumar P, Divatia JV, Sharma K. A prospective randomized controlled double-blind study comparing auscultation and lung ultrasonography in the assessment of double lumen tube position in elective thoracic surgeries involving one lung ventilation at a tertiary care cancer institute. *Korean J Anesthesiol* 2019;72:24-31.
13. Ramsingh D, Frank E, Haughton R, et al. Auscultation versus point-of-care ultrasound to determine endotracheal versus bronchial intubation: a diagnostic accuracy study. *Anesthesiology* 2016;124:1012-20.
14. Parab SY, Divatia JV, Chogle A. A prospective comparative study to evaluate the utility of lung ultrasonography to improve

- the accuracy of traditional clinical methods to confirm position of left sided double lumen tube in elective thoracic surgeries. *Indian J Anaesth* 2015;59:476-81.
15. Lichtenstein DA, Lascols N, Prin S, Mezière G. The “lung pulse”: an early ultrasound sign of complete atelectasis. *Intensive Care Med* 2003;29:2187-92.
 16. Breitzkreutz R, Seibel A, Zechner PM. Ultrasound-guided evaluation of lung sliding for widespread use? *Resuscitation* 2012;83:273-4.
 17. Lyon M, Walton P, Bhalla V, Shiver SA. Ultrasound detection of the sliding lung sign by prehospital critical care providers. *Am J Emerg Med* 2012;30:485-8.
 18. Sustić A, Protić A, Cicvarić T, Zupan Z. The addition of a brief ultrasound examination to clinical assessment increases the ability to confirm placement of double-lumen endotracheal tubes. *J Clin Anesth* 2010;22:246-9.
 19. Álvarez-Díaz N, Amador-García I, Fuentes-Hernández M, Dorta-Guerra R. Comparison between transthoracic lung ultrasound and a clinical method in confirming the position of double-lumen tube in thoracic anaesthesia. A pilot study. *Rev Esp Anestesiol Reanim* 2015;62:305-12.
 20. Saporito A, Lo Piccolo A, Franceschini D, et al. Thoracic ultrasound confirmation of correct lung exclusion before one-lung ventilation during thoracic surgery. *J Ultrasound* 2013;16:195-9.

Non-commercial use only